


IgG1-多聚体-对比图谱

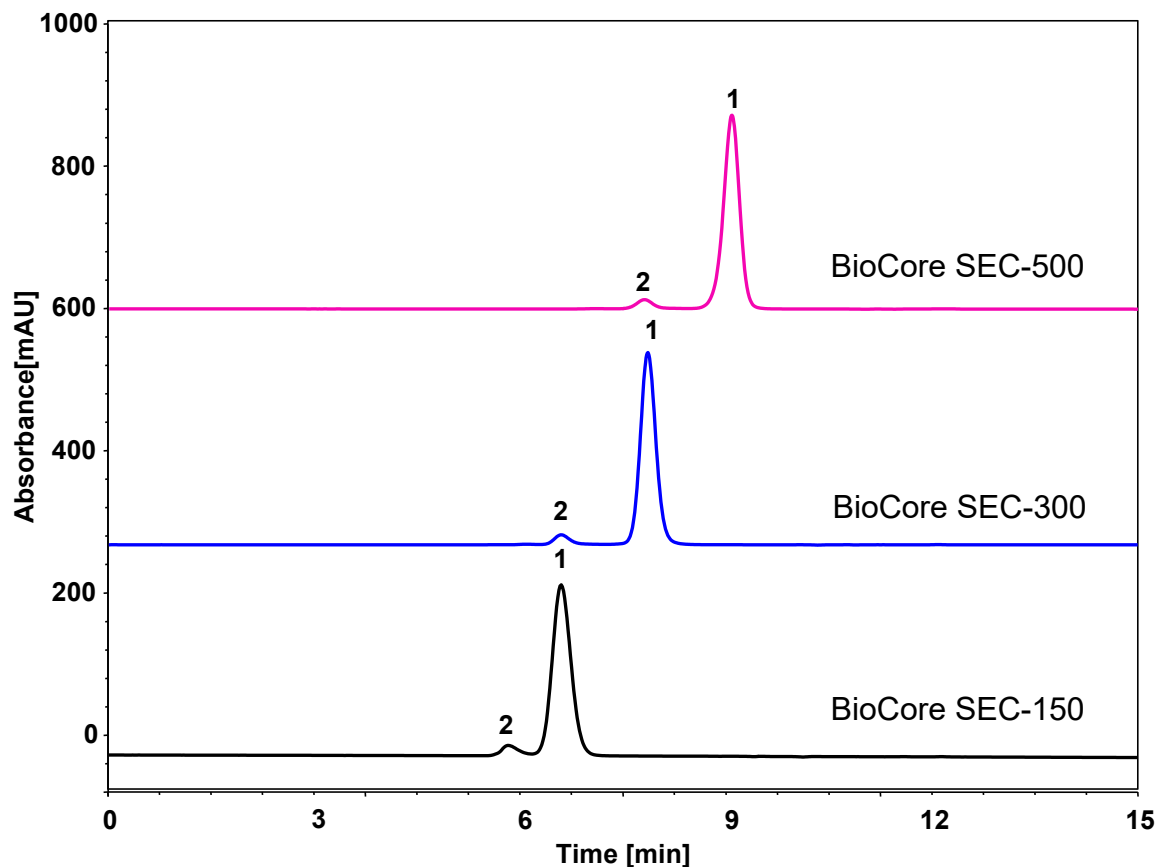

Columns: BioCore SEC-150, 5 μ m
 BioCore SEC-300, 5 μ m
 BioCore SEC-500, 5 μ m

Dimension: 4.6 \times 300 mm

Mobile Phase: 150 mM phosphate buffer, pH6.8

Flow Rate: 0.35 mL/min


Temperature: 30 $^{\circ}$ C

Injection: 5 μ L

Detection: UV 280 nm

Sample: IgG1 (2.6 mg/mL in water)

Peaks:
 1. IgG1
 2. IgG1 Aggregate



型号	流出时间 (IgG1)	分离度	峰纯度 (IgG1)
SEC-150	6.606 min	1.61	94.72 %
SEC-300	7.864 min	3.03	95.14 %
SEC-500	9.089 min	2.92	95.14 %