


ADC-疏水作用

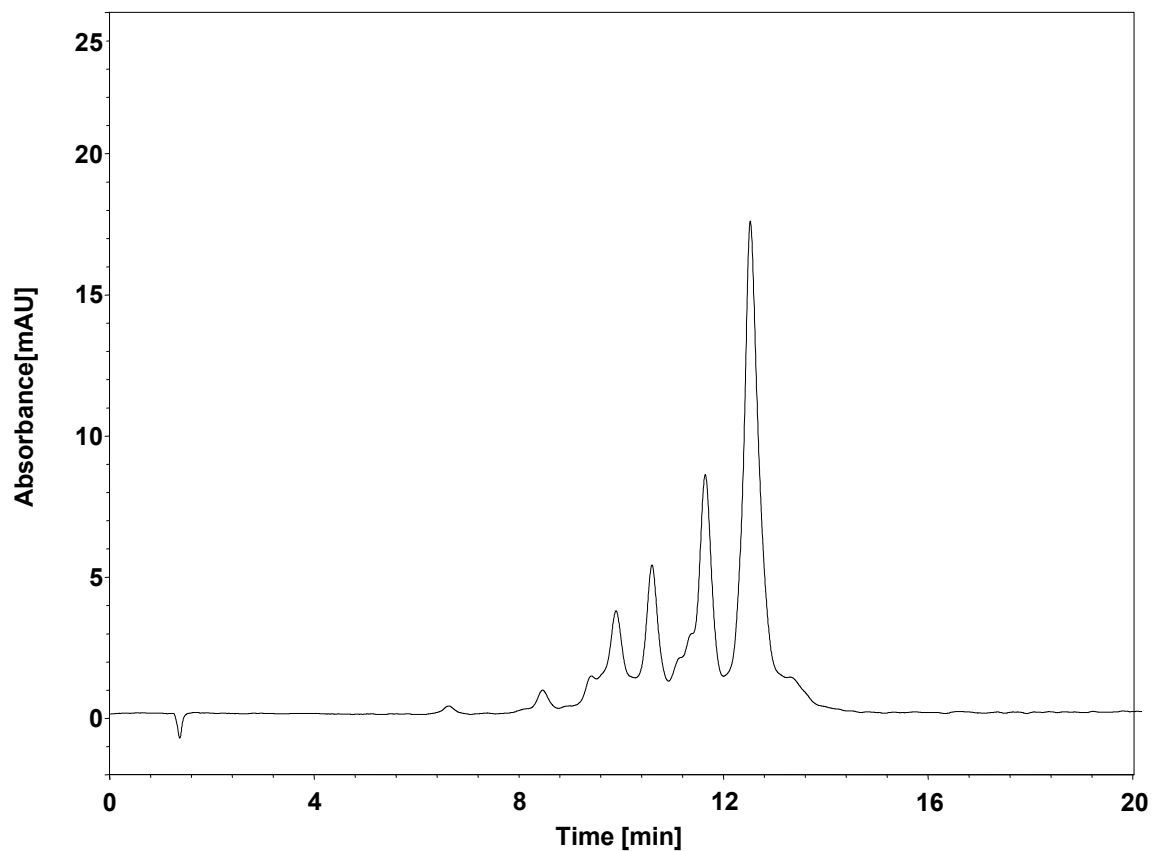

Column: BioCore HIC-Butyl, 5 μ m
Dimension: 4.6 \times 100 mm
Mobile Phase: A) 2.0 M $(\text{NH}_4)_2\text{SO}_4$ in 100 mM phosphate buffer, pH7.0
B) 100 mM phosphate buffer, pH7.0
C) Isopropanol

Gradient:	t (min)	%A	%B	%C
	0	59	41	0
	20	32	43	25
	20.1	0	75	25
	25	0	75	25
	25.1	59	41	0
	35	59	41	0

Flow Rate: 1.0 mL/min
Temperature: 30 $^\circ\text{C}$
Injection: 5 μL
Detection: UV 280 nm
Instrument: Agilent 1290 Infinity II (Bio)