


mRNA

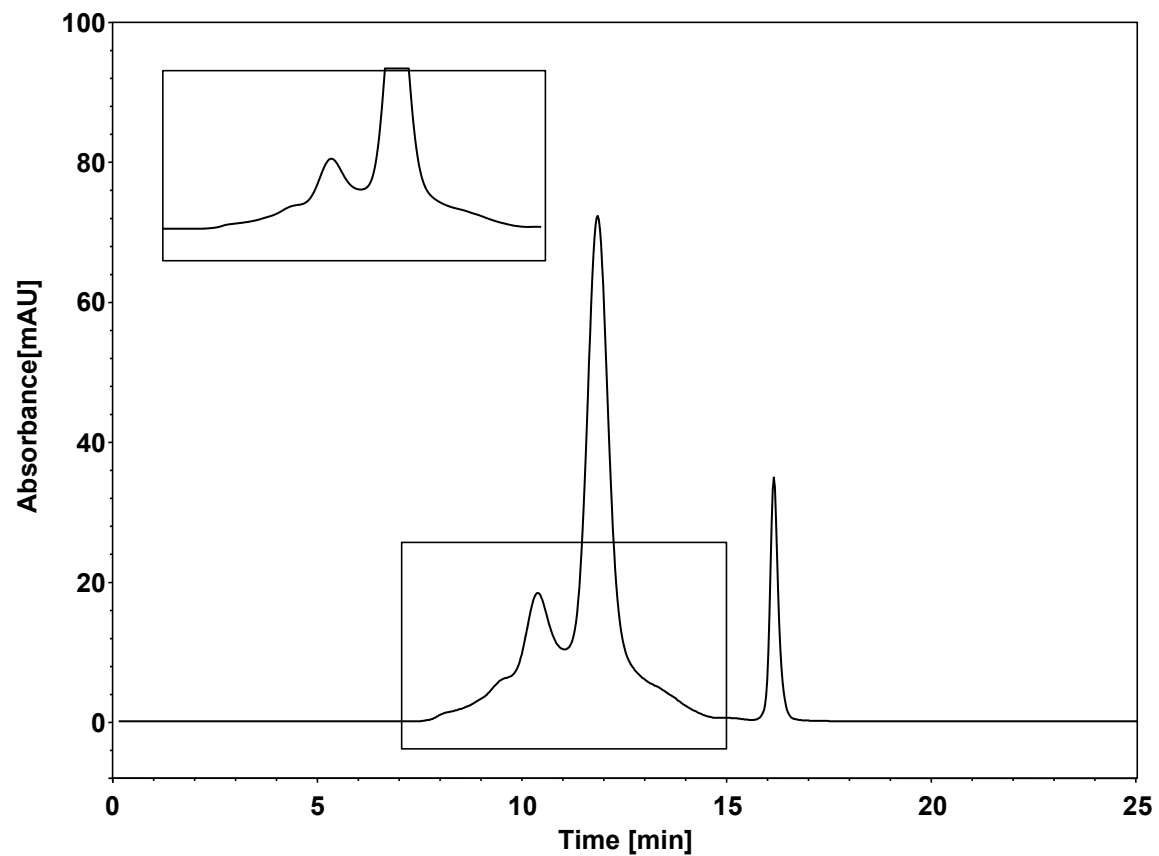

Column: BioCore SEC-1000, 5 μ m
Dimension: 7.8 \times 300 mm
Mobile Phase: 50 mM phosphate buffer, pH6.8
Flow Rate: 0.5 mL/min
Temperature: 25 $^{\circ}$ C
Injection: 3 μ L
Detection: UV 260 nm
Instrument: Agilent 1290 Infinity II (Bio)
Sample: mRNA (浓度: 1.52 mg/mL, 长度约: 2100~2200 nt)