


# ADC

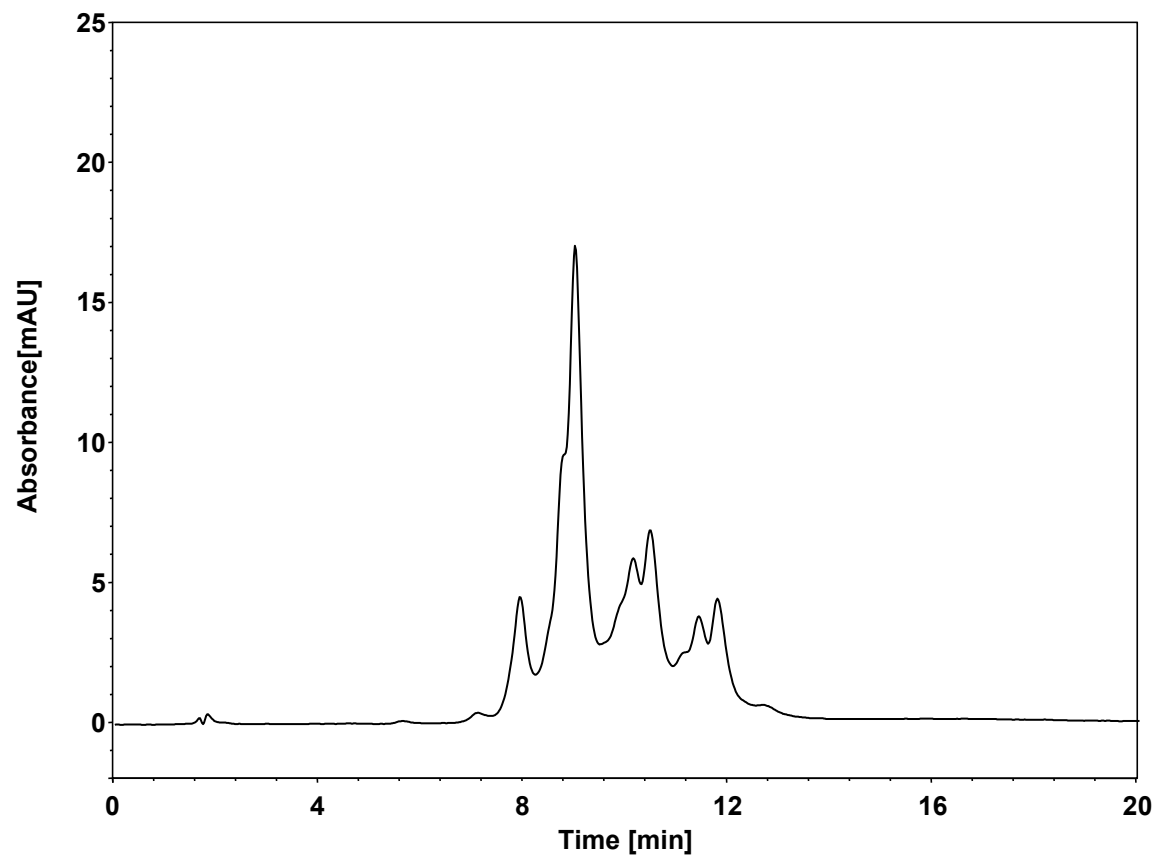

Column: BioCore HIC-Butyl, 5  $\mu\text{m}$   
Dimension: 4.6  $\times$  100 mm  
Mobile Phase: A) 7/93 v/v Isopropanol/2.0 M  $(\text{NH}_4)_2\text{SO}_4$  in 100 mM phosphate buffer, pH7.0  
B) 7/93 v/v Isopropanol/100 mM phosphate buffer, pH7.0

Gradient:

t (min)	%A	%B
0	90	10
1	90	10
20	0	100
21	90	10
30	90	10

Flow Rate: 0.8 mL/min  
Temperature: 30  $^\circ\text{C}$   
Injection: 14  $\mu\text{L}$   
Detection: UV 280 nm  
Instrument: Agilent 1290 Infinity II (Bio)  
Sample: ADC (1.78 mg/mL)