


ADC

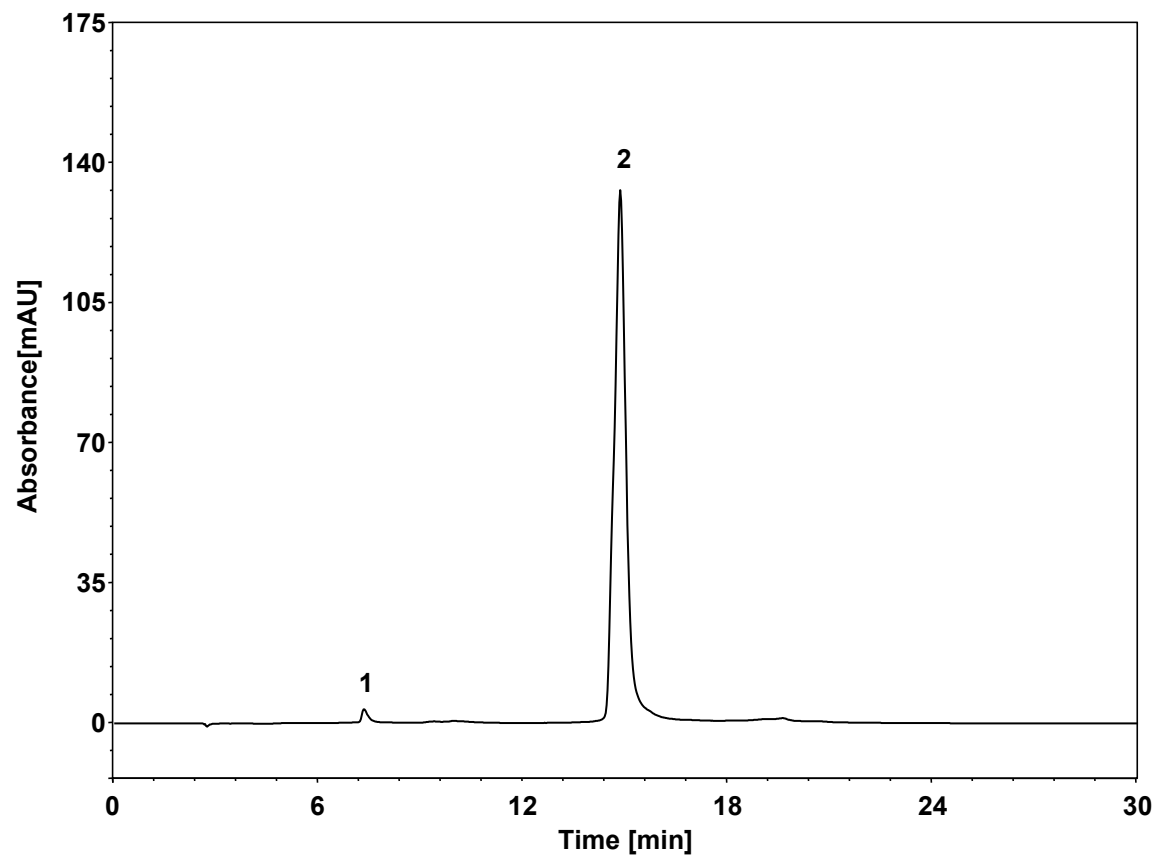

Column: BioCore HIC-Butyl, 5 μm
Dimension: 4.6 \times 100 mm
Mobile Phase: A) 1.5 M $(\text{NH}_4)_2\text{SO}_4$ in 50 mM phosphate buffer, pH7.0
B) 25/75 v/v Isopropanol/50 mM phosphate buffer, pH7.0

Gradient:	t (min)	%A	%B
	0	100	0
	1	100	0
	30	0	100
	35	0	100
	36	100	0
	45	100	0

Flow Rate: 0.5 mL/min
Temperature: 30 $^\circ\text{C}$
Injection: 5 μL
Detection: UV 280 nm
Instrument: Agilent 1290 Infinity II (Bio)
Sample: ADC (20 mg/mL)
Peaks:
1. 裸抗
2. ADC